


13/11/1967 (F)
Indication : AIMAGIOMA

CAP [dB/m]
IQR
84
MEDIAN
217

E [kPa]
MEDIAN
8.5
IQR
1.7
IQR/med.
20%

Exam XL (Liver)
Valid measurements : 10
Total measurements : 11

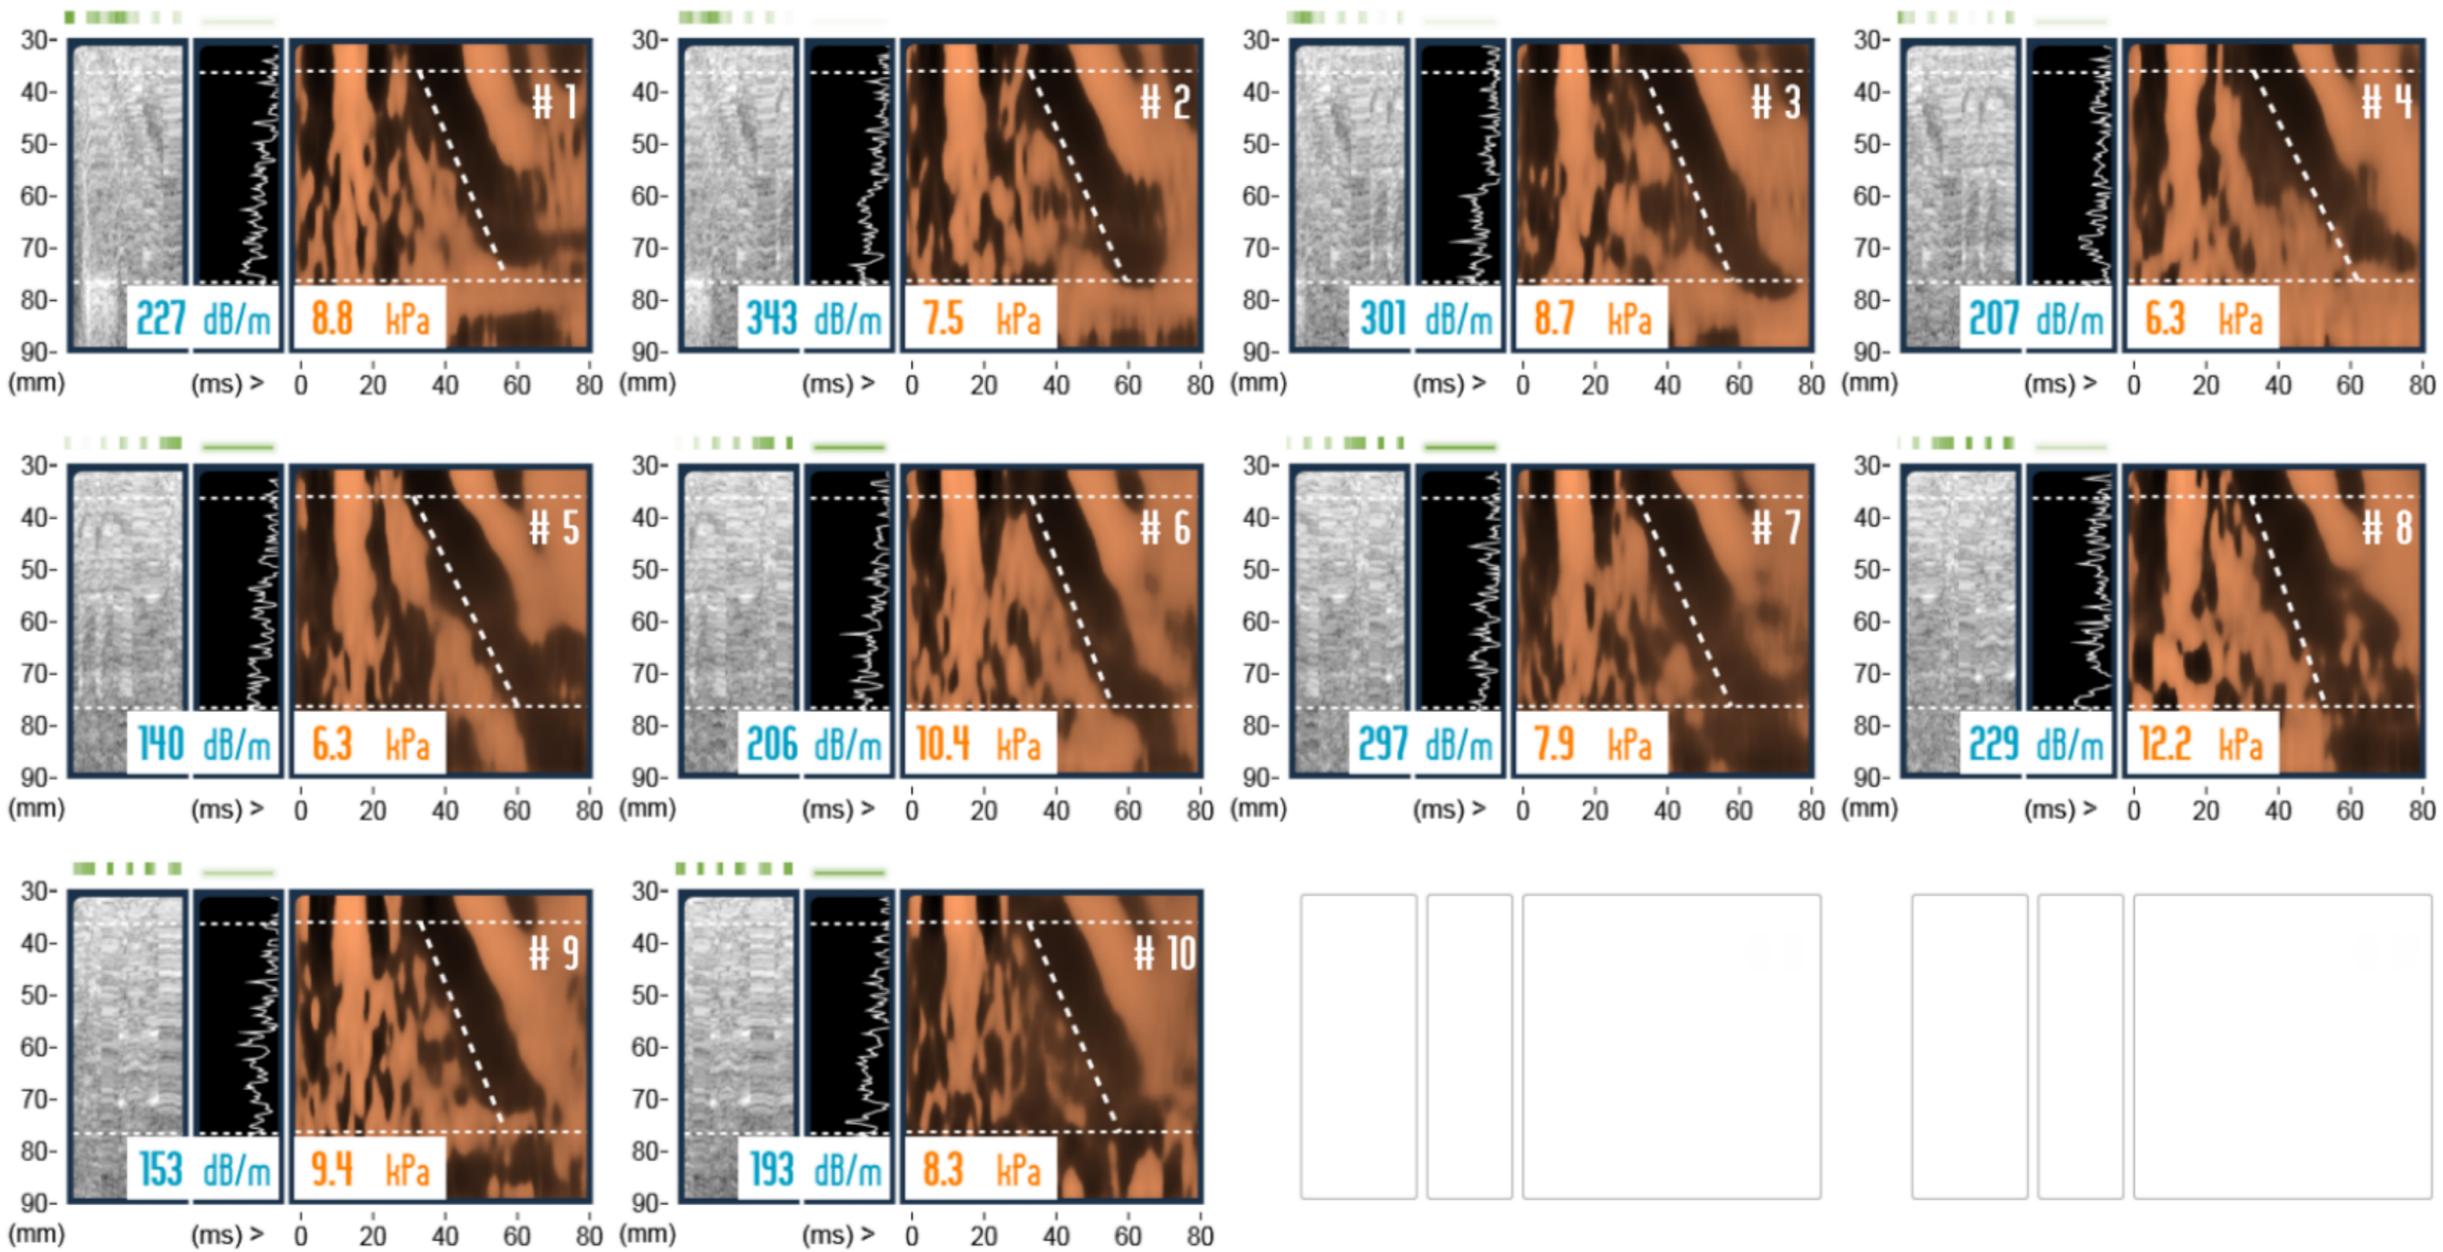

Comments :

FibroScan 530 Compact (SN:F80024) - Probe XL (SN:90893) - G3.1

FibroScan® is a medical device intended as an aid for the management of patients with liver disease. Measurements should be performed by a certified operator. The values obtained must be interpreted by a physician experienced in dealing with liver disease, taking into account the complete medical records of the patient, the number of valid measurements and their dispersion. Probes must be calibrated according to the manufacturer's recommendations.